

SAR, Absorbed & Incident Power Density with DASY8

# APPLICATION NOTE

Updated Interim Procedures (Version 6.0) for 6 - 10 GHz

# Demonstrating Compliance of Devices Operating between 6 – 10 GHz: Updated Interim Procedures (Version 6.0)

## 1 Introduction

With the opening of the Unlicensed National Information Infrastructure (U-NII) bands above 6 GHz, procedures for assessing the *peak spatial incident Power Density (psPD)* compliance testing in the reactive near-field, i.e., at distances smaller than  $\lambda/5$ , are required. SPEAG and the IT'IS Foundation (Zurich, Switzerland) have joined forces in a research collaboration to develop novel methods for compliance testing of devices operating between 6 – 10 GHz. A first report was published in October 2020 and provides a workaround for distance smaller than  $\lambda/5$  [6] using the developed Plane-to-Plane Phase Reconstruction (PTP-PR) Algorithm used in Module mmWave V2.x. However, the required measurement effort and the resulting uncertainties were not satisfactory.

Recently, SPEAG and IT'IS achieved a breakthrough by developing a novel equivalent source reconstruction (ESR) algorithm, that models an unknown and inaccessible transmitter as a set of distributed known auxiliary sources below the surface of the device enclosure. The positions, amplitudes, and phases of these sources are then determined to optimally reconstruct the measured near-fields. As a result, the transmitters inside any enclosure can be replaced with these equivalent sources in any radiation problem, including exposure assessment scenarios. The novel method has been submitted for publication [9] and a first implementation is now available in DASY8 Module mmWave V3.0 and Sim4Life V7.0.

In parallel to this development, regulators have started to use the dosimetric quantity *peak spatial Absorbed Power Density (psAPD)* instead of the incident psPD [8] as a limit. Within a short time, the International Electrotechnical Commission (IEC) reacted and developed the Publicly Available Specifications (PAS) entitled "Conversion Method of Specific Absorption Rate (SAR) to Absorbed Power Density for the Assessment of Human Exposure to Radio Frequency Electromagnetic Fields from Wireless Frequency Electromagnetic Fields from Wireless Devices in Close Proximity to the Head and Body-Frequency Range of 6 GHz to 10 GHz."

This application note describes practical guidelines and testing procedures for demonstrating compliance of devices transmitting at frequencies between 6 – 10 GHz. They are consistent with the interim procedures introduced by the Federal Communications Commission (FCC) during the Telecommunications Certification Body (TCB) workshop in October 2020.

The measurement procedures described in this Application Note also apply to DASY6 users.

## 2 Hardware & Software Requirements

### 2.1 SAR / APD

Required Component	Compatible Model	Remarks
<b>Hardware</b>		
Probe	EX3DV4	Additional calibration required for 6 – 10 GHz (frequency validity extended to $\pm 700$ MHz)
Phantoms	SAM & ELI	–
Tissue Simulating Liquid	HBBL600-10000V6	–
Dipoles	D6.5GHzV2, D7GHzV2 D8GHzV2 and D9GHzV2	Calibrated for HSL at respective frequencies
<b>Software</b>		
Software	Module SAR V16.2+	Includes advanced extrapolation and APD

Table 1.1: Hardware and software components required for SAR / APD measurements at 6 – 10 GHz

### 2.2 PD

Required Component	Compatible Model	Remarks
<b>Hardware</b>		
Probe	EUmmWVx	Calibrated from 0.75 – 110 GHz
Phantom	mmWave	–
Verification Source	5G Verification Source 10 GHz	Calibrated at 10 GHz
<b>Software</b>		
Software	Module mmWave V3.0+	Includes PD evaluations with equivalent source reconstruction

Table 1.2: Hardware and software components required for PD measurements at 6 – 10 GHz

## 3 Interim Procedures for FCC Radiofrequency Exposure Evaluations

The interim procedure for FCC radiofrequency (RF) exposure evaluations of U-NII 6–7 GHz band portable devices have been made available during the TCB workshop in October 2020. The procedure is summarized below:

- evaluate SAR / APD with DASY8 Module SAR V16.2 or higher according to [3]. The configurations to be tested are defined in the relevant Knowledge Database (KDB). The peak spatial averaged SAR (psSAR) and the peak spatial averaged absorbed Power Density (psAPD) are reported.
- for the configuration with the highest SAR / APD, evaluate the PD with DASY8 Module mmWave V3.0 or higher.

## 4 SAR / APD Measurements with DASY8 Module SAR

This section describes how to perform SAR / APD measurements according to the IEC/IECC 62209-1528:2020 [3]. It is the first step of the interim procedure for FCC RF exposure evaluations of U-NII 6–7 GHz band portable devices. The procedure is very similar to the one used for devices operating below 6 GHz.

### 4.1 Tissue Simulating Liquid (TSL)

Frequency (MHz)	Permittivity ( $\epsilon$ )	Conductivity (S/m)
6500	34.5	6.07
7000	33.9	6.65
8000	32.7	7.84
9000	31.6	9.08

Table 1.3: Dielectric target values for Head Simulating Liquid (HSL) media according to [3]

SPEAG's head broad band liquid 600–10000 (HBBL600–10000Vx) meets the outlined dielectric parameters (Table 1.3) with a maximum deviation of less than  $\pm 10\%$ .

### 4.2 Probe Calibration

At frequencies above 6 GHz, the probe conversion factor is valid over a large frequency range (typically  $\pm 700$  MHz) and the dielectric parameters of the TSL are changing rapidly with the frequency. In the 6 - 10 GHz frequency range, the dielectric parameters ( $\epsilon, \sigma$ ) range for which the probe conversion factor is valid is adjusted to the measurement frequency as described in Equation 1.1:

$$\begin{aligned} 0.9 * (\sigma + 1.23 * \Delta_f) < \sigma < 1.1 * (\sigma + 1.23 * \Delta_f) \\ 0.9 * (\epsilon - 1.18 * \Delta_f) < \epsilon < 1.1 * (\epsilon - 1.18 * \Delta_f) \end{aligned} \quad (1.1)$$

where:

$\sigma$  = conductivity of the TSL in S/m

$\epsilon$  = permittivity of the TSL

$\Delta_f$  = measurement frequency - calibration frequency in GHz

### 4.3 System Performance Check and System Validation

For system check and validation purposes, four dipoles have been developed: D6.5GHzV2, D7GHzV2, D8GHzV2, and D9GHzV2 (see Figure 1.1). The spacer, which has a nominal thickness of 5 mm  $\pm$ 0.1 mm in the 6 – 10 GHz frequency range, is integral to the antenna. The updated numerical psSAR / psAPD target values for these dipoles are summarized in Table 1.4.

Freq (MHz)	Shell (mm)	psSAR1g (W/kg)	psSAR8g (W/kg)	psSAR10g (W/kg)	psAPD <sub>1cm<sup>2</sup></sub> <sup>SAR</sup> (W/m <sup>2</sup> )	psAPD <sub>4cm<sup>2</sup></sub> <sup>SAR</sup> (W/m <sup>2</sup> )	psAPD <sub>1cm<sup>2</sup></sub> <sup>sqr</sup> (W/m <sup>2</sup> )	psAPD <sub>4cm<sup>2</sup></sub> <sup>sqr</sup> (W/m <sup>2</sup> )
6500	2.0	298	64.9	52.8	$2.98 \cdot 10^3$	$1.29 \cdot 10^3$	$3.32 \cdot 10^3$	$1.30 \cdot 10^3$
7000	2.0	286	59.7	48.7	$2.86 \cdot 10^3$	$1.19 \cdot 10^3$	$3.15 \cdot 10^3$	$1.20 \cdot 10^3$
8000	2.0	273	54.6	44.5	$2.73 \cdot 10^3$	$1.09 \cdot 10^3$	$2.93 \cdot 10^3$	$1.09 \cdot 10^3$
9000	2.0	240	49.0	39.3	$2.40 \cdot 10^3$	$0.98 \cdot 10^3$	$2.55 \cdot 10^3$	$0.96 \cdot 10^3$

Table 1.4: Updated numerical target psSAR / psAPD derived from the SAR (psAPD<sup>SAR</sup>), and the directly determined numerical psAPD<sup>sqr</sup> target values for the 6 – 10 GHz system-check dipoles at the nominal distance to the Flat phantom. The psAPD<sup>sqr</sup> is evaluated using a rotating square as averaging area as specified in [4] whereby the numerical modeling uncertainty is 0.34 dB (the deviations compared to the previous values are less than 0.17 dB). Calibrated values are provided in the calibration certificate.



Figure 1.1: Two of the four dipoles (i.e., D7GHzV2 and the D9GHzV2) used for system performance checks in the frequency range between 6 – 10 GHz

System performance checks are performed with the dipole which operates at the closest frequency of the measurement frequency following the procedures defined in [3], see Section A.2 / A.5.

System validation is performed using the procedures of [3] except for the measurement with a 2 cm transverse offset from the feed-point, as the exposure is too localized to provide meaningful results at that offset, i.e., local SAR  $\ll$  -20 dB of peak SAR (see Section A.3.5 b) of [3]).

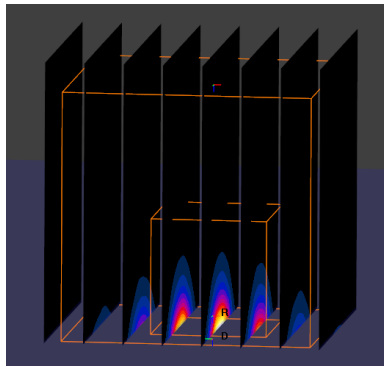


Figure 1.2: SAR Distribution of a D6.5GHzV2 system dipole

## 4.4 Measurement Procedure

The measurement procedure used to assess the SAR below 6 GHz remains valid for frequencies up to 10 GHz. The following scans are performed:

- a Fast Area Scan to define the most appropriate location for the power reference point used in the subsequent scans
- an Area Scan to determine the location of the maximum SAR
- a Zoom Scan anchored at the maximum location of the Area Scan. SPEAG recommends the use of the *Smart Zoom Scan* as the measurement grid will be refined on the fly to fulfill the Zoom Scan grid resolution described in [3].

For frequencies above 6 GHz, the DASY8 Module SAR Zoom Scan results provide the *psSAR* averaged over 1g, 8g and 10 g (*psSAR*1g/8g/10g) as well as the absorbed *psAPD* averaged over  $1\text{cm}^2$  and  $4\text{cm}^2$  (*psAPD*1 $\text{cm}^2$ /4 $\text{cm}^2$ ). Both quantities must be reported to the regulators.

## 4.5 Experimental Uncertainty for APD Evaluations

### 4.5.1 APD System Check and Validation

The uncertainty of the experimental evaluation of the *psAPD* of Table 1.5 is assessed according to [3, 5] for DASY8. The expanded standard uncertainty of the experimental evaluations is  $\pm 29.0\%$  ( $1\text{cm}^2$ ) and  $\pm 28.8\%$  ( $4\text{cm}^2$ ), which corresponds to 1.1 dB. The same sources can be used for system check and validation as the numerical target values have been computed in accordance with the requirements for validation of [3]. Note that the SAR assessment uncertainty for 8 g is the same as for 10 g.

## 4.6 APD Assessments

The uncertainty of the experimental evaluation of the *psAPD* of Table 1.5 is assessed according to [3, 5] for DASY8. The expanded standard uncertainty of the experimental assessment of any device under test (DUT) is 1.2 dB.

<b>Uncertainty Budget for psSAR / psAPD System Check</b> (Frequency band: 6 – 10 GHz range)								
Symbol	Error Description	Uncert.	Prob. Dist.	Div.	$c_i$ (1g) / (1 cm <sup>2</sup> )	$c_i$ (8g/10g) / (4 cm <sup>2</sup> )	Std. Unc. (1g) / (1 cm <sup>2</sup> )	Std. Unc. (8g/10g) / (4 cm <sup>2</sup> )
psSAR	Module SAR V16.2 (Table 6.2.3)	±13.1%	N	1	1	1	±13.1%	±13.0%
PDC	Power Density Conversion	±13.5%	R	$\sqrt{3}$	$0.8^D$	$0.8^D$	±6.2%	±6.2%
$u(\Delta SAR)$	Combined Uncertainty						±14.5%	±14.4 %
U	<b>Expanded Uncertainty</b>						±29.0%	±28.8%

Table 1.5: Uncertainty of a system validation (6 – 10 GHz) using DASY8 Module SAR V16.2 or higher according to [5]. The RF ambient noise uncertainty has been reduced to ±1.0, considering input power levels are ≥250 mW. All listed error components have  $v_{eff}$  equal to ∞.

**Footnote details:** <sup>D</sup> valid for system check dipoles.

<b>Uncertainty Budget for psSAR / psAPD Assessments</b> (Frequency band: 6 – 10 GHz range)								
Symbol	Error Description	Uncert.	Prob. Dist.	Div.	$c_i$ (1g) / (1 cm <sup>2</sup> )	$c_i$ (8g/10g) / (4 cm <sup>2</sup> )	Std. Unc. (1g) / (1 cm <sup>2</sup> )	Std. Unc. (8g/10g) / (4 cm <sup>2</sup> )
psSAR	Module SAR V16.2 (Table 6.3.3)	±14.2/13.9%	N	1	1	1	±14.2%	±13.9%
PDC	Power Density Conversion	±13.5%	R	$\sqrt{3}$	1	1	±7.8%	±7.8%
$u(\Delta SAR)$	Combined Uncertainty						±16.2%	±15.9 %
U	<b>Expanded Uncertainty</b> <i>in dB</i>						±32.4%	±31.9%
							±1.2 dB	±1.2 dB

Table 1.6: Uncertainty of psAPD assessments for devices operating between 6 – 10 GHz using DASY8 Module SAR V16.2 or higher according to [5]. All listed error components have  $v_{eff}$  equal to ∞.

## 5 PD Measurements with DASY8 Module mmWave

The incident PD must be measured for the test configuration producing the highest SAR value. It involves the following procedure:

- perform a system performance check at 10 GHz
- measure the DUT at the required test distances

*Note that there is no need to adjust the incident psPD results since the total uncertainty is below 2 dB for test distances larger than  $\lambda/25$ .*

### 5.1 System Performance Check

System checks can be performed with the [5G Verification Source 10 GHz](#) (see Figure 1.3). The measurement procedure is described in Section A.3 of [4].

For system performance checks at 10 GHz, it is recommended to use a grid step of  $0.125\lambda$  and a grid extend of 60 mm.

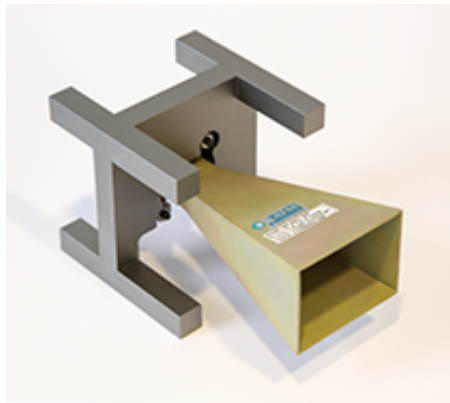


Figure 1.3: Horn Antenna used for system check at 10 GHz

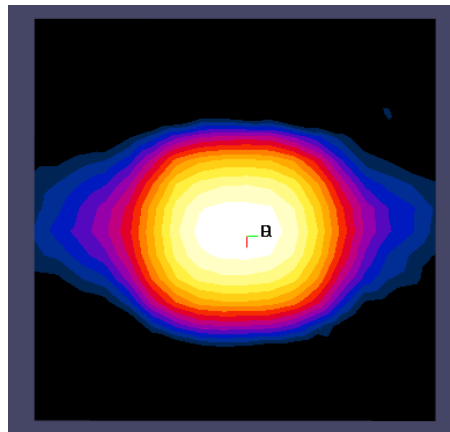


Figure 1.4: Measured electric field distribution for the 10 GHz Horn Antenna at 10 mm from the opening

## 5.2 Incident PD Assessment

For measurements in the 6 – 10 GHz range, the grid step to be used as function of the test distance is given by:

$$l_{grid} = \begin{cases} 1.25d & \text{for } d < \lambda/10 \\ \lambda/8 & \text{for } d \geq \lambda/10 \end{cases} \quad (1.2)$$

with  $d$ : the test distance as fraction of  $\lambda$ .

In addition, the measurement grid extent  $\nu_{grid}$  should not be less than  $2\lambda$ , or  $16 \times 16$  grid points.

Before the measurement is started, please check that the ESR algorithm is enabled. To do this, log into DASY8 Module mmWave as Administrator, then go to Application Preferences » Post Processing Settings. Under Reconstruction Algorithm, set the Reconstruction mode to Hybrid. In this mode, the ESR will be automatically used at frequencies up to 10 GHz. At higher frequencies, the PTP-PR will be used.



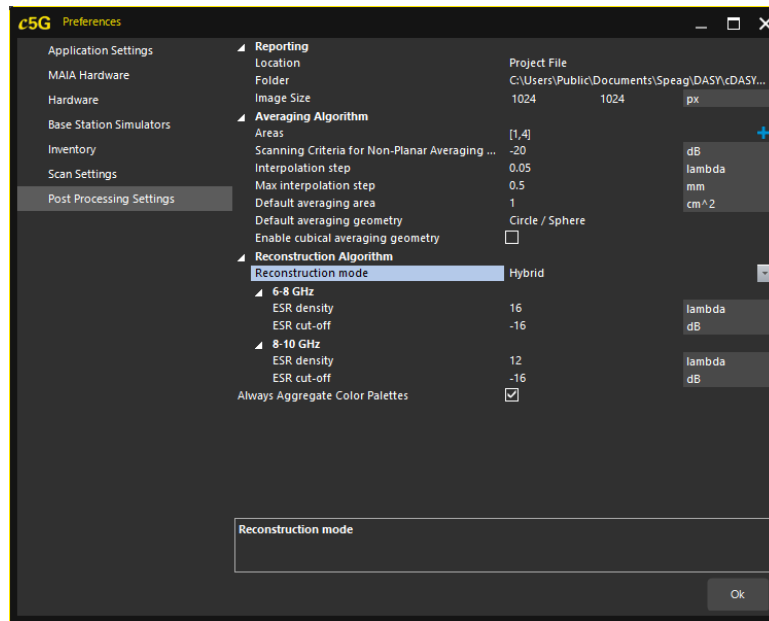


Figure 1.5: Selection of the ESR as Reconstruction Algorithm at 6 – 10 GHz


## 6 Conclusion

This application note illustrates how DASY8 can be used for FCC RF exposure evaluations of U-NII 6–7 GHz band portable devices according to the interim procedures introduced during the TCB workshop in October 2020. It also contains all information on how to assess APD using the latest ESR method [9]. This method will be generalized and optimized for all sources in DASY8 Module mmWave V3.2 which will also simplify evaluation of transmitters operating above 10 GHz.

# Bibliography

- [1] IEEE PC95.1/D3.3 *Draft Standard for Safety Levels with Respect to Human Exposure to Electric, Magnetic and Electromagnetic Fields, 0 Hz to 300 GHz*, 2019
- [2] ICNIRP, *Draft ICNIRP Guidelines for limiting exposure to time-varying electric, magnetic and electromagnetic fields (up to 300 GHz)*, Health Physics, 2019
- [3] IEC/IEEE 62209-1528:2020, *Measurement procedure for the assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-worn wireless communication devices - Part 1528: Human models, instrumentation and procedures (Frequency range of 4 MHz to 10 GHz)*, October 2020.
- [4] IEC/IEEE 63195-1 ED1, *Assessment of power density of human exposure to radio frequency fields from wireless devices in close proximity to the head and body (Frequency range of 6 GHz to 300 GHz) - Part 1: Measurement procedure*, CFDIS, September 2021.
- [5] IEC PAS, *Conversion method of specific absorption rate to absorbed power density for the assessment of human exposure to radio frequency electromagnetic fields from wireless devices in close proximity to the head and body - Frequency Range of 6 GHz to 10 GHz*, Final Draft, January 2022
- [6] Kristian Cujia, Leif Klysner, Arya Fallahi, Andreas Christ, Niels Kuster, *Solutions for Testing Compliance of Devices Operating between 6 – 10 GHz with DASY6*, preliminary report, October 2020.
- [7] E. Carrasco, D. Colombi, K. R. Foster, M. C. Ziskin, Q. Balzano, Exposure Assessment of Portable Wireless Devices above 6 GHz. *Radiat Prot Dosimetry*. 2019 Jun 1;183(4):488-495. doi: 10.1093/rpd/ncy177. PMID: 30289490.
- [8] Supplementary Procedure for Assessing Specific Absorption Rate & Absorbed Power Density Compliance of Portable Devices in the 6 GHz Band (5925-7125 MHz), ISED SPR-APD, Issue 1, November 2021.
- [9] Kristian Cujia, Arya Fallahi, Sylvain Reboux, Niels Kuster, *Experimental Exposure Evaluation from the Very Close Near- to the Far-Field using a Multiple-Multipole Source Reconstruction Algorithm*, IEEE Transactions on Antennas and Propagation (revision submitted February 2022; copy of the manuscripts are available on special request).

# Appendix

	Project	Document Name	Rev.
	I20211013	IRR-20211013	6

**Numerical Target Values of  
System Check and Validation Dipole Antennas  
6.5 GHz to 9 GHz**

	Name	Function	Date	Signature
<b>Author</b>	Andreas Christ	External Consultant	Oct 21, 2021	
<b>Approval</b>	Niels Kuster	Quality Manager. Director	Oct 21, 2021	

**Numerical Target Values of  
System Check and Validation Dipole Antennas  
6.5 GHz to 9 GHz**

conducted by

**Andreas Christ, Erdem Ofli and Theodore Samaras**

Zurich, October 21<sup>th</sup>, 2021

The names of IT<sup>IS</sup> and any of the researchers involved may be mentioned only in connection with statements or results from this report. The mention of names to third parties other than certification bodies may be done so only after written approval from Prof. Dr. N. Kuster.

**Confidential**

## Executive Summary

Recently, a method was proposed to obtain the peak spatial average absorbed power density (psAPD) at the surface of a lossy medium from the evaluation of the peak spatial average SAR. The method was validated using dipole antennas from 6.5 GHz to 9.0 GHz as well as dipole and slot array antennas. The target values were obtained for a circular averaging area. As the final draft of [1] specifies a rotating square as averaging area, the psAPD values were reevaluated. The deviations of the reevaluated results with respect to the previous ones using the circular averaging area are found to be less than 0.04 dB. The maximum deviations from the results converted from psSAR are 0.43 dB, which are in-line with the values reported in [2]. The expanded numerical standard uncertainty has been evaluated as 0.34 dB. The expanded experimental standard uncertainty for the APD assessment of the system check dipoles has been reassessed to 1.1 dB.

---

## **Contents**

<b>1 Objectives</b>	<b>4</b>
<b>2 Methods</b>	<b>4</b>
2.1 Numerical Model and Simulations . . . . .	4
2.2 Evaluation of the psAPD Based on the psSAR . . . . .	4
<b>3 Results</b>	<b>5</b>
<b>4 Numerical Uncertainty for Target Values</b>	<b>7</b>
<b>5 Experimental Uncertainty for APD System Check</b>	<b>8</b>
<b>6 Conclusions</b>	<b>8</b>
<b>References</b>	<b>9</b>

## 1 Objectives

The objective of this short report is to provide validated numerical target results for the absorbed power densities for the dipoles for system performance check and validation operating at 6.5, 7, 8 and 9 GHz that are compliant with the performance specifications of the standards [3, 4]. The dipoles are evaluated numerically, and the peak average spatial absorbed power density (psAPD) at the phantom bottom is evaluated following [1, 4]. The numerical evaluations are complemented by measurements using the dosimetric assessment system DASY8 (SPEAG, Zurich, Switzerland). The numerical uncertainty is evaluated by adapting the methods of [1, 5], and the assessment of the experimental uncertainty follows [4].

## 2 Methods

### 2.1 Numerical Model and Simulations

Numerical models of the dipoles for system check and validation specified for the frequencies from 6.5 GHz to 9.0 GHz in [3] are generated based on the original drawings. These models consider the feed of the dipole through the dipole leg made of coaxial semi-rigid. The models are simulated at a flat phantom with a lossless dielectric shell ( $\epsilon_r = 3.7$ ) and the dielectric spacer according to the manufacturer's specifications. All simulations are carried out using the finite-difference time-domain method [6] and the simulation platform Sim4Life, Versions 5.0.0 and 6.2.1 (ZMT Zurich MedTech AG (ZMT), Switzerland).

The impact of the numerical parameters, such as mesh resolution, simulated time, distance to absorbing boundary conditions, etc., was adapted iteratively until convergence of the numerical results was reached. The peak spatial average specific absorption rate (psSAR) was evaluated according to [5]. The peak spatial average absorbed power density (psAPD) at the tissue surface was integrated over circular averaging areas of  $1 \text{ cm}^2$  and  $4 \text{ cm}^2$  following the dimensions given in [7, 8] using the implementation of Sim4Life Version 5.0.0. The circular averaging area was used as the averaging algorithm of the final draft of [1] had not been finalized at the time of the evaluation. Additional results applying the rotating square as averaging area that is defined in the final draft of [1] have been evaluated with Sim4Life Version 6.2.1 and added to this report (Section 3).

### 2.2 Evaluation of the psAPD Based on the psSAR

The efficient evaluation of the psAPD from psSAR results has recently been demonstrated in [2]. Conversion factors (CF) can be applied to calculate the psAPD from the psSAR provided that the psSAR is evaluated in a cube with the same surface area as the averaging area for the psAPD. Conversion factors of  $\text{CF}_{1\text{g}} = 10 \text{ kg/m}^2$  and  $\text{CF}_{8\text{g}} = 20 \text{ kg/m}^2$  to calculate the  $1 \text{ cm}^2$  and  $4 \text{ cm}^2$  from the 1 g psSAR and the 8 g psSAR, respectively. The uncertainty of this conversion has been quantified with less than 0.55 dB [2]. Based on this method, JWG12 of the IEC TC106 has initiated the development of a Publicly Available Specification for the assessment of the psAPD using SAR measurements for the frequency range from 6 GHz to 10 GHz.



### 3 Results

Table 1 shows the simulated results of for the psAPD of the dipole antennas for the frequency range from 6.5 GHz to 9.0 GHz in comparison to the values obtained from the psSAR according to [2]. The maximum deviation of the converted results from the simulated ones is 0.47 dB. The psSAR results according to [5] are given in Table 2.

Updated psAPD results that have been determined applying the rotating square as averaging area as specified in [1] are given in Table 3. Differences between these and the results evaluated with the circular averaging volume (Table 1) are less than 0.04 dB. The deviations with respect to the values converted from the psSAR are also within 0.47 dB. In general, a reduction of the uncertainty of the evaluation of the psAPD by conversion from the psSAR according to [4] can be observed when the frequency increases, which is due to the higher penetration depth. I.e., an increasing part of the electromagnetic energy is absorbed in the psSAR averaging volume.

The experimental results are within the mutual uncertainty of the applied numerical and experimental methods (Sections 4 and 5). They are not reported here.

Table 1: psAPD evaluated from the psSAR according to [2,4] and integrated from the surface power density of the numerical simulation results

frequency /(GHz)	converted from psSAR		simulated, circular		deviations	
	1 cm <sup>2</sup> /(kW/m <sup>2</sup> /W)	4 cm <sup>2</sup> /(kW/m <sup>2</sup> /W)	1 cm <sup>2</sup> /(kW/m <sup>2</sup> /W)	4 cm <sup>2</sup> /(kW/m <sup>2</sup> /W)	1 cm <sup>2</sup> /(dB)	4 cm <sup>2</sup> /(dB)
6.5	2.98	1.29	3.32	1.30	0.47	0.02
7.0	2.86	1.19	3.15	1.20	0.41	0.00
8.0	2.73	1.09	2.93	1.09	0.31	-0.01
9.0	2.40	0.98	2.55	0.96	0.27	-0.07

Table 2: psSAR evaluated according to [5] for the same dipoles. The values in brackets shows the values reported earlier in [3]. The deviation of up to 0.17 dB corresponds to the numerical modeling uncertainty of 0.34 dB.

frequency /(GHz)	1 g psSAR /(W/kg)	8 g psSAR /(W/kg)	10 g psSAR /(W/kg)
6.5	298.4	64.6	52.8
7.0	286.0 (275.0)	59.7	48.7 (47.0)
8.0	273.1	54.6	44.5
9.0	239.5 (243.0)	49.0	39.3 (40.0)

Table 3: psAPD evaluated using a rotating square as averaging area specified in [1]

frequency /(GHz)	converted from psSAR		simulated, rotating square		deviations	
	1 cm <sup>2</sup> /(kW/m <sup>2</sup> /W)	4 cm <sup>2</sup> /(kW/m <sup>2</sup> /W)	1 cm <sup>2</sup> /(kW/m <sup>2</sup> /W)	4 cm <sup>2</sup> /(kW/m <sup>2</sup> /W)	1 cm <sup>2</sup> /(dB)	4 cm <sup>2</sup> /(dB)
6.5	2.98	1.29	3.30	1.29	0.43	0.00
7.0	2.86	1.19	3.12	1.19	0.38	-0.01
8.0	2.73	1.09	2.92	1.09	0.29	-0.03
9.0	2.40	0.98	2.54	0.96	0.25	-0.08

## 4 Numerical Uncertainty for Target Values

The uncertainty of the numerical psAPD of Table 3 is estimated with methods that generally follow [1, 5] and have been adapted to the particular requirements of the numerical setup of the dipole antennas and the phantom. The uncertainty budget is given in Table 4. The expanded standard uncertainty of the numerical evaluations is  $\pm 8\%$  (0.34 dB).

As the numerical uncertainty is assumed to increase for higher frequencies, the uncertainty assessment is carried out for the dipole and phantom setup for 9 GHz. For the evaluation of the uncertainty components, the deviations of the  $1 \text{ cm}^2$  and  $4 \text{ cm}^2$  psAPD are evaluated separately. The maximum deviation is reported in Table 4 to achieve a conservative estimate of the uncertainty. In detail, the uncertainty components are evaluated as follows:

- **Mesh resolution:** The maximum mesh steps of the dipole antenna and of the area in which the psSAR and the psAPD are averaged are reduced to 50% of their default values.
- **Positioning:** The distance between dipole and phantom is changed by  $\pm 1$  mesh step.
- **Phantom dimensions:** The overall length and width of the phantom are increased by 25% with respect to their default dimensions.
- **Shorting cylinder:** The length of the shorting cylinder of the dipole has been modified by  $\lambda/4$  and terminated both in free space and in the absorbing boundary conditions of the computational domain.
- **Absorbing boundary conditions:** The computational domain has been increased by  $\lambda/4$  in all directions with respect to its original dimensions.
- **Power budget:** The deviation of the sum of the radiated and total dissipated power from the antenna feedpoint power is reported.
- **Convergence:** The total simulated time has been reduced by 30% with respect to the reference simulation. The deviation is reported.
- **Power density averaging:** [4] does not specify a method for the calculation of the psAPD. The values in Table 4 are calculated by evaluating the  $\text{psPD}_{n+}$  at the interface of the tissue simulant and the phantom shell according to [1]. This calculation is affected by interpolation uncertainties due to the finite mesh spacing. These interpolation uncertainties are assessed by comparing  $\text{psPD}_{n+}$  to  $\text{psPD}_{\text{tot}+}$ . An average value for the observed deviations is reported.

Numerical Uncertainty Budget						
Error Description	Uncert. value	Prob. Dist.	Div.	$(c_i)$	Std. Unc. (max. of $1 \text{ cm}^2$ and $4 \text{ cm}^2$ )	$(v_i)$ $v_{eff}$
Mesh resolution phantom	2.0%	N	1	1	2.0%	$\infty$
Mesh resolution dipole	0.1%	N	1	1	0.1%	$\infty$
Positioning (dist. dipole - phantom)	4.0%	R	$\sqrt{3}$	1	2.3%	$\infty$
Phantom dimensions	0.2%	R	$\sqrt{3}$	1	0.1%	$\infty$
Shorting cylinder	0.1%	N	1	1	0.1%	$\infty$
Absorbing boundary conditions	0.3%	R	$\sqrt{3}$	1	0.2%	$\infty$
Power budget	2.7%	N	1	1	2.7%	$\infty$
Convergence	0.3%	R	$\sqrt{3}$	1	0.2%	$\infty$
Power density averaging	6.6%	N	1	1	6.6%	$\infty$
Combined Std. Uncertainty					$\pm 4 \%$	$\infty$
<b>Expanded STD Uncertainty</b>					<b><math>\pm 8 \%</math> (0.34 dB)</b>	$\infty$

Table 4: Numerical uncertainty budget of the evaluation of the psAPD (Table 3) adapted from [1, 5].

## 5 Experimental Uncertainty for APD System Check

The uncertainty of the experimental evaluation of the psAPD of Table 5 is assessed according to [3, 4] for DASY8/6. The expanded standard uncertainty of the experimental evaluations is  $\pm 29.0\%$  (1 g) and  $\pm 28.8\%$  (8 g), which corresponds to 1.1 dB .

<b>Uncertainty Budget for APD System Check</b> (Frequency band: 6 GHz–10 GHz range)								
Symbol	Error Description	Uncert. value	Prob. Dist.	Div.	$c_i$ (1 g)	$c_i$ (10 g)	Std. Unc. (1 g)	Std. Unc. (8 g)
psSAR	Module SAR V16.2 (Table 6.2.3)	$\pm 13.1\%$	N	1	1	1	$\pm 13.1\%$	$\pm 13.0\%$
PDC	Power Density Conversion	$\pm 13.5\%$	R	$\sqrt{3}$	$0.8^D$	$0.8^D$	$\pm 6.2\%$	$\pm 6.2\%$
$u(\Delta SAR)$	Combined Uncertainty						$\pm 14.5\%$	$\pm 14.4\%$
U	<b>Expanded Uncertainty</b>						$\pm 29.0\%$	$\pm 28.8\%$

Table 5: Uncertainty of a system validation (6 GHz–10 GHz) using DASY8/6 Module SAR V16.2 or higher according to [4]. The RF ambient noise uncertainty has been reduced to  $\pm 1.0$ , considering input power levels are  $\geq 250$  mW. All listed error components have  $v_{eff}$  equal to  $\infty$ .

**Footnote details:**  $^D$  valid for system check dipoles.

## 6 Conclusions

The  $1 \text{ cm}^2$  and  $4 \text{ cm}^2$  psAPD of the dipole antennas for system check and validation for frequencies from 6.5 GHz to 9.0 GHz [3] has been reevaluated applying the average algorithm for the power density using a rotating square area as specified in [1]. The new results are compared to those converted from the numerical psSAR evaluation proposed in [2]. The deviations with respect to the previous evaluation using a circular averaging area are found to be less than 0.04 dB. The maximum deviations from the results converted from psSAR are 0.47 dB, which corresponds to the values reported in [2], previously.

The numerical uncertainty has been evaluated as 0.34 dB, and the experimental uncertainty has been evaluated as 1.1 dB. It should be noted that one of the major contributing factors of the numerical uncertainty budget is the power density averaging according to [1]. This method has originally been specified for the averaging of the incident power density in free space. It is expected that the numerical uncertainty due to the averaging can be reduced when [4] specifies an averaging algorithm with improved interpolation at the dielectric interface of the phantom shell and the tissue simulant.

## References

- [1] IEC/IEEE 63195-2, *DRAFT Assessment of power density of human exposure to radio frequency fields from wireless devices in close proximity to the head and body - Part 2: Computational procedures (Frequency range of 6 GHz to 300 GHz)*, International Electrotechnical Commission (IEC), IEC Technical Committee 106, Geneva, Switzerland, 2020.
- [2] Theodoros Samaras, Andreas Christ, and Niels Kuster, “Compliance assessment of the epithelial or absorbed power density below 10 GHz using SAR measurement systems”, *Bioelectromagnetics*, vol. 42, no. 6, pp. 484–490, September 2021.
- [3] IEC/IEEE 62209-1528, “Measurement procedure for the assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-worn wireless communication devices — Human models, instrumentation and procedures (Frequency range of 4 MHz to 10 GHz)”, 2020.
- [4] IEC/IEEE, *DRAFT Publicly Available Specification: Conversion method of specific absorption rate to absorbed power density for the assessment of human exposure to radiofrequency electromagnetic fields from wireless devices in close proximity to the head and body — (Frequency range of 6 GHz to 10 GHz)*, International Electrotechnical Commission (IEC), IEC Technical Committee 106, Geneva, Switzerland, 2022.
- [5] IEC/IEEE 62704-1, *Recommended Practice for Determining the Spatial-Peak Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices, 30 MHz - 6 GHz — Part 1: General Requirements for using the Finite Difference Time Domain (FDTD) Method for SAR Calculations*, International Electrotechnical Commission (IEC), IEC Technical Committee 106, Geneva, Switzerland, 2017.
- [6] K. S. Yee, “Numerical solution of initial boundary value problems involving Maxwell’s equations in isotropic media”, *IEEE Transactions on Antennas and Propagation*, vol. 14, pp. 585–589, 1966.
- [7] International Commission on Non-Ionizing Radiation Protection et al., “Guidelines for limiting exposure to electromagnetic fields (100 kHz to 300 GHz)”, *Health Physics*, vol. 118, no. 5, pp. 483–524, 2020.
- [8] IEEE C95.1, *Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 0 Hz to 300 GHz*, IEEE Standards Department, International Committee on Electromagnetic Safety, The Institute of Electrical and Electronics Engineers, Inc. 3 Park Avenue, New York, NY 10016-5997, USA, Oct. 2019.